




Enable Successful Library Updates with Wireless Pumps

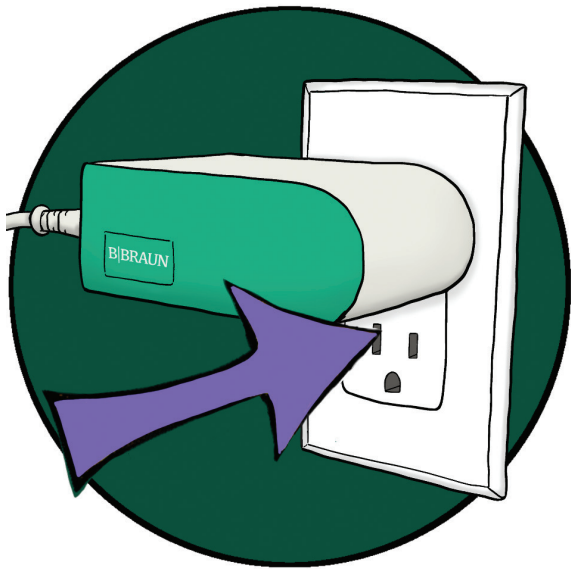

PLUGGED IN

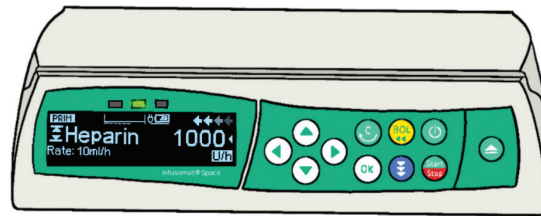


INFUSING

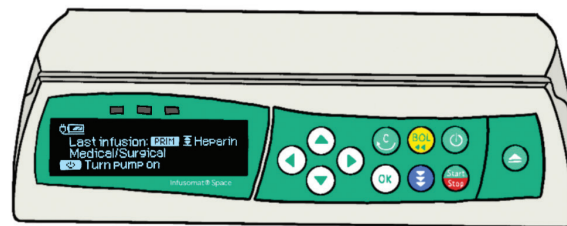


OFF

▶ **DRUG LIBRARY RECEIVED**

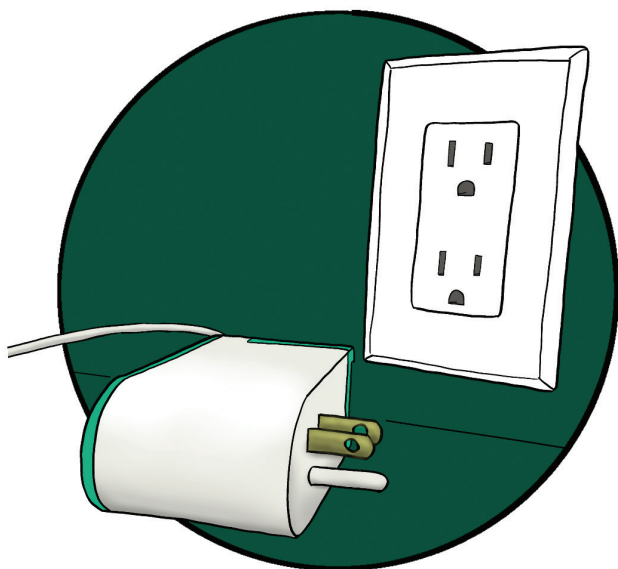


UNPLUGGED

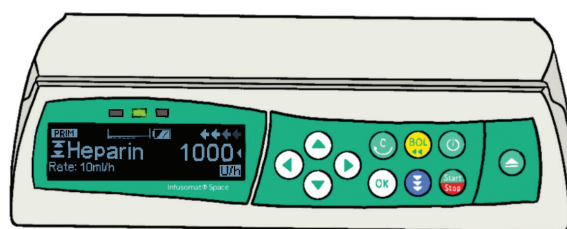


INFUSING

▶ **DRUG LIBRARY RECEIVED**

But better keep the pump plugged in to ensure full charge of the battery at all time.

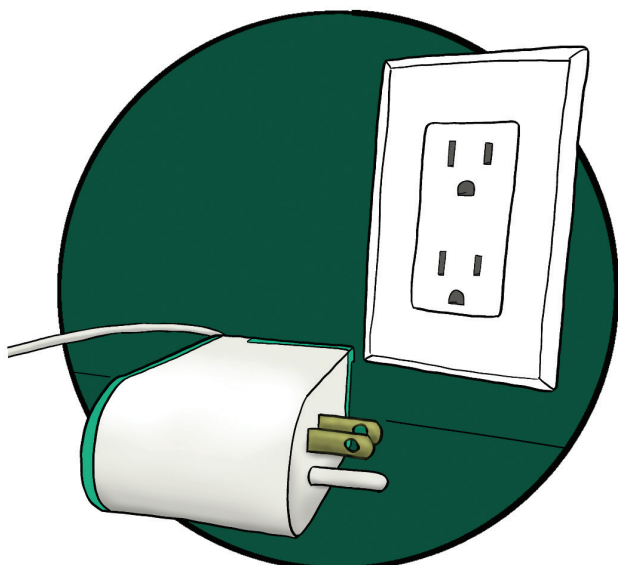

UNPLUGGED

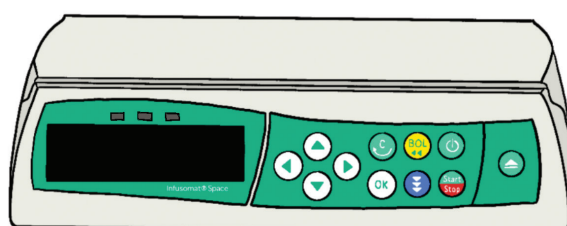

OFF

▶ **DRUG LIBRARY NOT RECEIVED**

The pump will receive the Drug Library when back on A/C power or when it is powered on.